



Talisman Flotta Terminal

OIW EX1000 & Laboratory
Correlation

Data Supplied Courtesy Of
Talisman UK






March 2007

Average Difference for Month= 1.0039PPM




169 Sample March 07

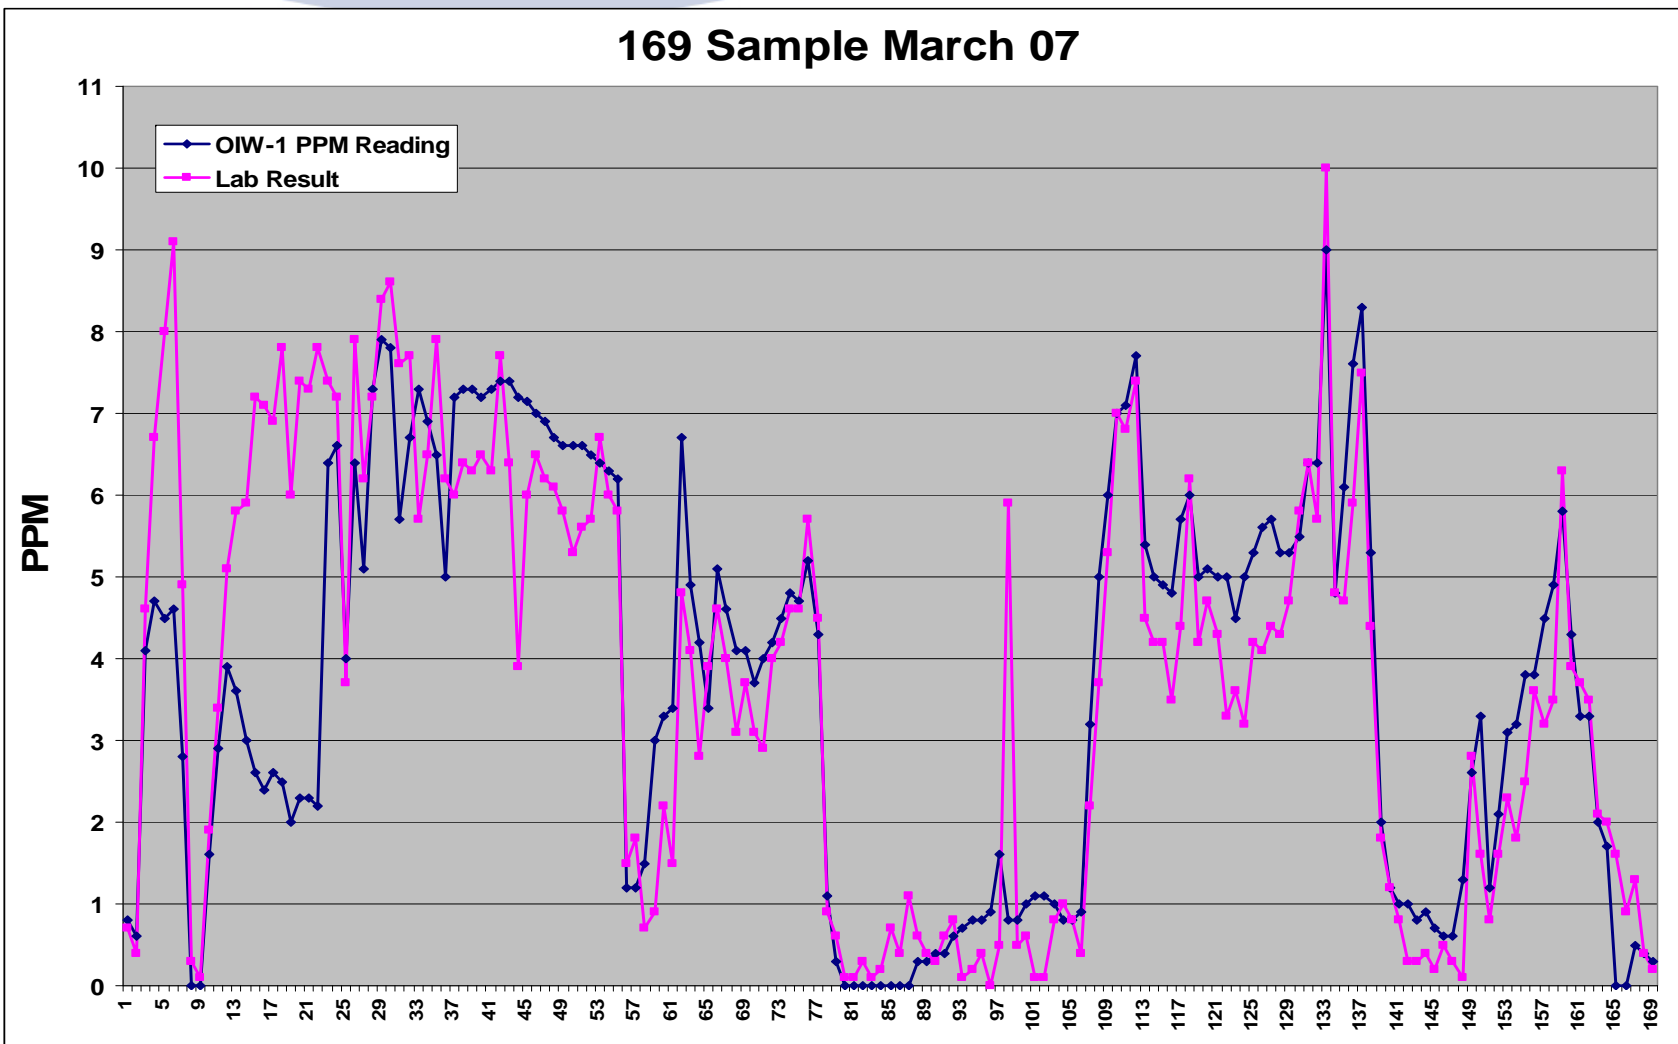



April 2007


Average Difference for Month= 0.8345PPM

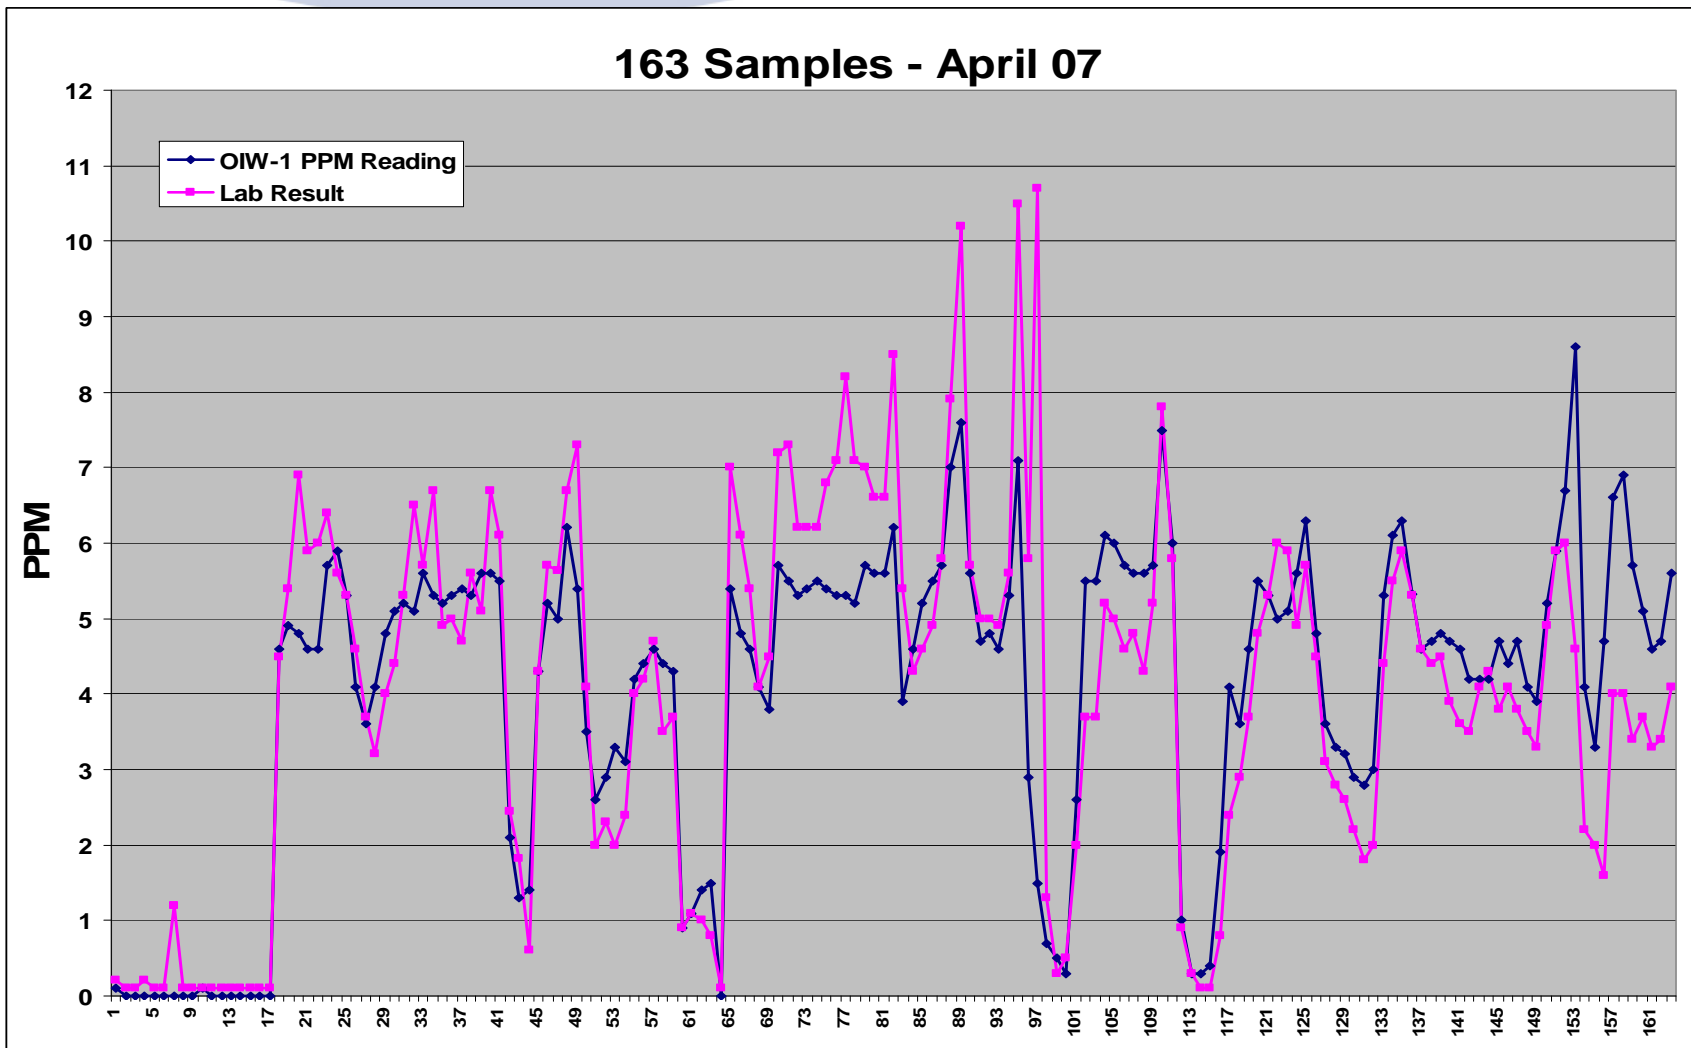



May 2007

Average Difference for Month= 0.8591PPM

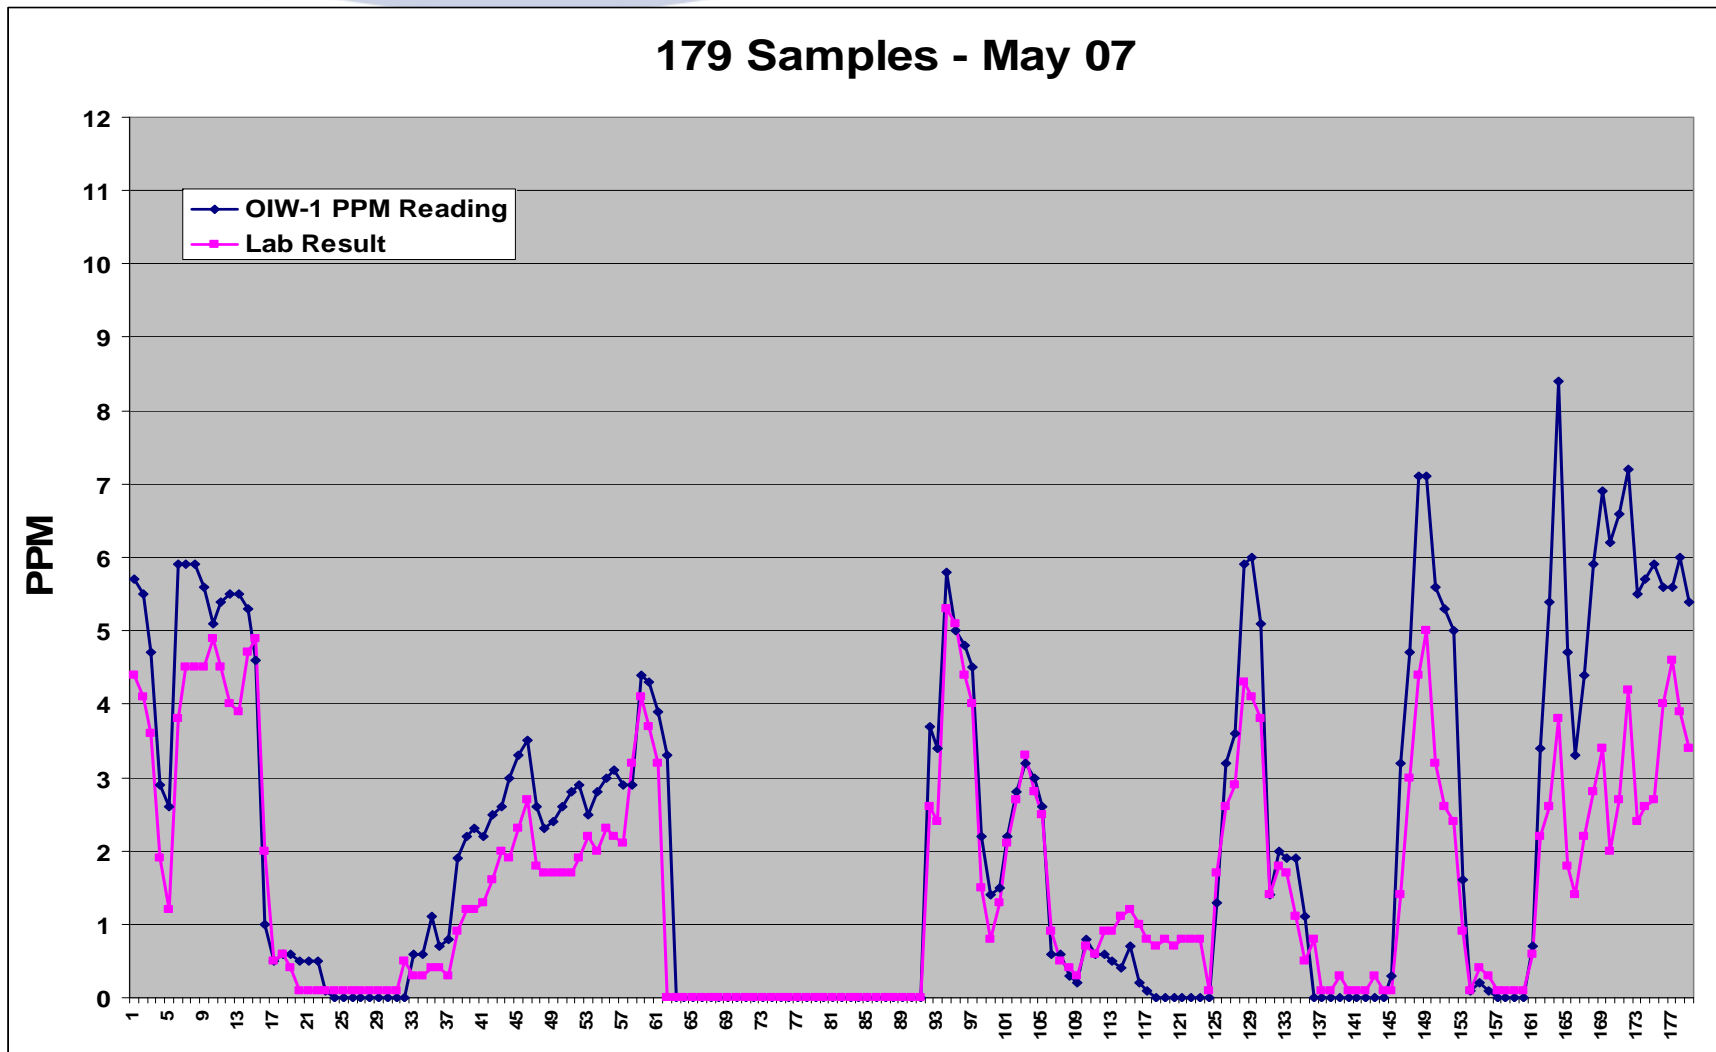



December 2007

Average Difference for Month= 0.34PPM

